



WYATT
TECHNOLOGY

6300 Hollister Avenue
Santa Barbara, CA 93117

Tel: +1 (805) 681-9009
Fax: +1 (805) 681-0123
Web: www.wyatt.com

Pierce BSA
(Lot No:RG236150)

Certificate of Analysis

Pierce Bovine Serum Albumin (BSA)



Wyatt p/n: P8401-02

Lot Number: RG236150

Manufactured by: Thermo Scientific

Expires: 8/9/17

Storage: 4°C

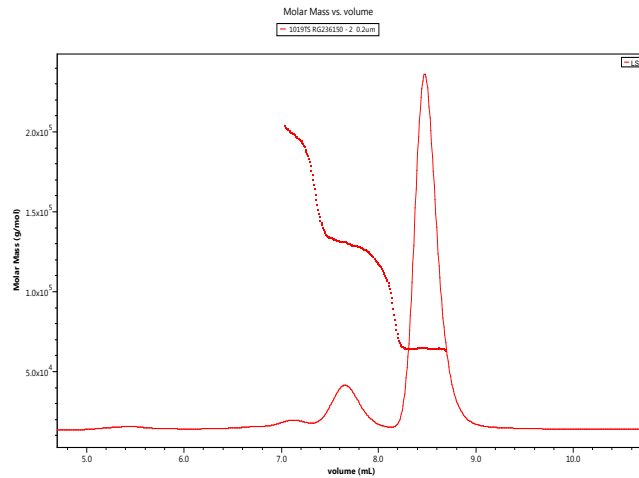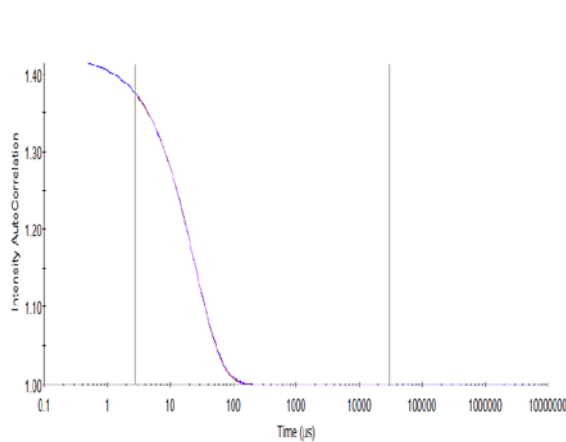

Standard characterization data by Wyatt DynaPro NanoStar or Plate Reader:

Solution filtered through 0.02 µm Anotop filter

R_h (from Cumulant) = (3.9 ± 0.1) nm; R_h (from Regularization) = (4.0 ± 0.1) nm

Solution filtered through 0.2 µm Anotop filter

R_h (from Cumulant) = (4.3 ± 0.1) nm; R_h (from Regularization) = (4.2 ± 0.2) nm

Standard characterization data by Wyatt MALS detector following SEC separation (WTC-030S5 with PBS at 0.5 mL/min):

(Solution filtered through 0.02 µm Anotop filter)

Monomer% = (91.4 ± 0.3); M_w (including aggregates) = (73.6 ± 0.1) kDa

(Solution filtered through 0.2 µm Anotop filter)

Monomer% = (90.9 ± 0.8); M_w (including aggregates) = (74.6 ± 0.9) kDa

Certification: Sigrid Kuebler

Date: 8/10/16

Dr. Sigrid Kuebler, Director of Customer Service