



WYATT
TECHNOLOGY

6300 Hollister Avenue
Santa Barbara, CA 93117

Tel: +1 (805) 681-9009
Fax: +1 (805) 681-0123
Web: www.wyatt.com

Pierce BSA
(Lot No:RI236148)

Certificate of Analysis

Pierce Bovine Serum Albumin (BSA)



Wyatt p/n: P8401-02

Lot Number: RI236148

Manufactured by: Thermo Scientific

Expires: Dec. 1, 2017

Storage: 4°C

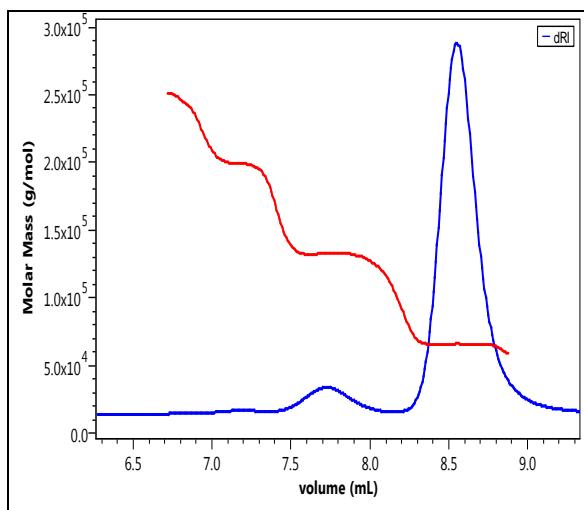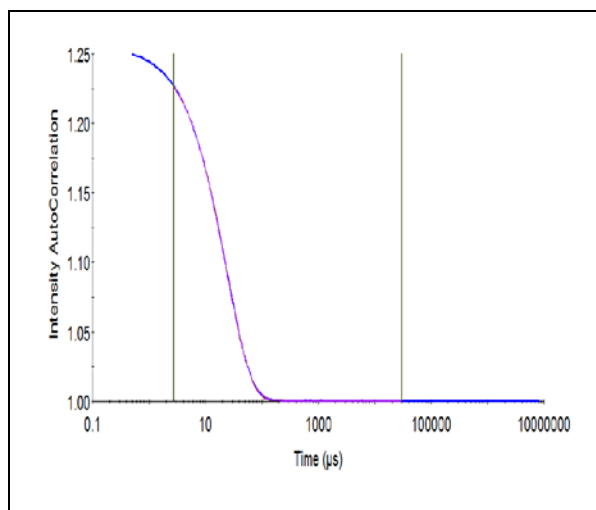

Standard characterization data by Wyatt DynaPro NanoStar or Plate Reader:

Solution filtered through 0.02 µm Anotop filter

R_h (from Cumulant) = (3.8 ± 0.1) nm; R_h (from Regularization) = (3.9 ± 0.1) nm

Solution filtered through 0.2 µm Anotop filter

R_h (from Cumulant) = (4.1 ± 0.1) nm; R_h (from Regularization) = (3.9 ± 0.1) nm

Standard characterization data by Wyatt MALS detector following SEC separation (WTC-030S5 with PBS at 0.5 mL/min):

(Solution filtered through 0.02 µm Anotop filter)

Monomer% = (90.3 ± 0.1); M_w (including aggregates) = (72.3 ± 0.2) kDa

(Solution filtered through 0.2 µm Anotop filter)

Monomer% = (89.7 ± 0.1); M_w (including aggregates) = (75.3 ± 0.2) kDa

Certification: Michelle Chen

Date: Nov. 21, 2016

Dr. Michelle Chen, Director of Analytical Services