



WYATT
TECHNOLOGY

6330 Hollister Avenue
Santa Barbara, CA 93117

Tel: +1 (805) 681-9009
Fax: +1 (805) 681-0123
Web: www.wyatt.com

Pierce BSA
(Lot No:TI269558)

Certificate of Analysis

Pierce Bovine Serum Albumin (BSA)



Wyatt p/n: P8401-02

Lot Number: TI269558

Manufactured by: Thermo Scientific

Expires: 11/26/2019

Storage: Room Temperature

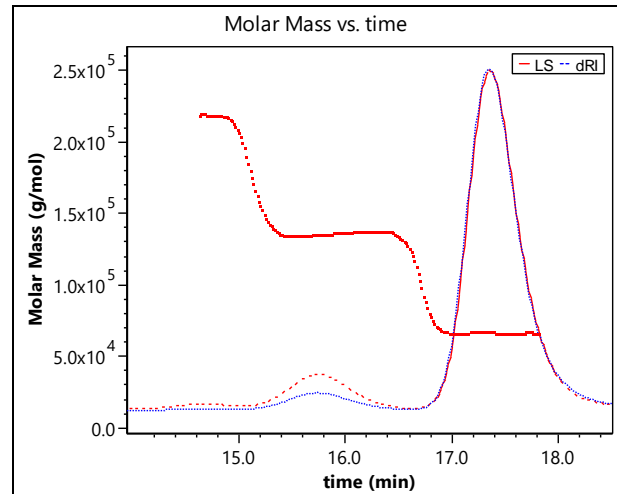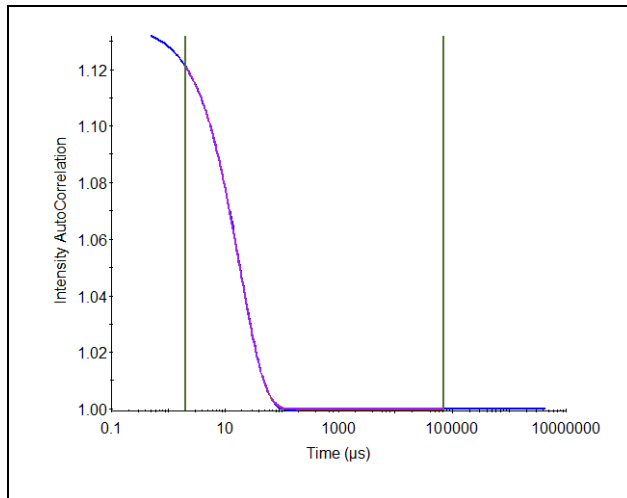

Standard characterization data by Wyatt DynaPro NanoStar or Plate Reader:

Solution filtered through 0.02 µm Anotop filter

R_h (from Cumulant) = (3.7 ± 0.1) nm; R_h (from Regularization) = (3.8 ± 0.1) nm

Solution filtered through 0.2 µm Anotop filter

R_h (from Cumulant) = (4.0 ± 0.1) nm; R_h (from Regularization) = (4.0 ± 0.2) nm

Standard characterization data by Wyatt MALS detector following SEC separation (WTC-030S5 with PBS at 0.5 mL/min):

(Solution filtered through 0.02 µm Anotop filter)

Monomer% = 92.8 ± 0.1 ; M_w (including aggregates) = (73.0 ± 0.2) kDa

(Solution filtered through 0.2µm Anotop filter)

Monomer% = 92.7 ± 0.6 ; M_w (including aggregates) = (73.0 ± 0.6) kDa

Certification: _____ **Michelle Chen** _____

Date: _____ 11/26/2018 _____