



WYATT TECHNOLOGY

6330 Hollister Avenue
Santa Barbara, CA 93117

Tel: +1 (805) 681-9009
Fax: +1 (805) 681-0123
Web: www.wyatt.com



Pierce BSA (Lot No:UD269568)

Certificate of Analysis

Pierce Bovine Serum Albumin (BSA)

Wyatt p/n: P8401-02
Lot Number: UD269568

Manufactured by: Thermo Scientific
Expires: 6/12/2020
Storage: Room Temperature

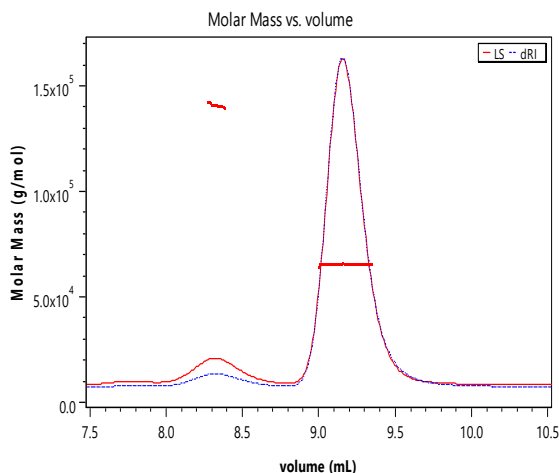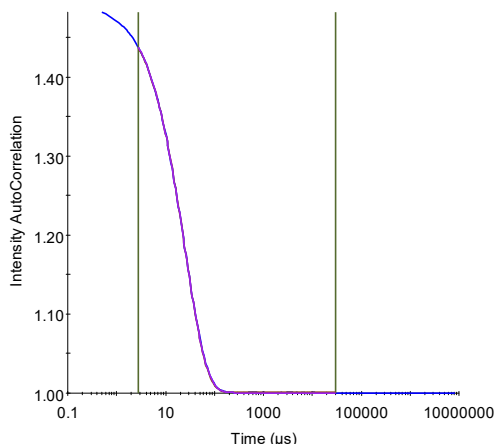

Standard characterization data by Wyatt DynaPro NanoStar or Plate Reader:

Solution filtered through 0.02 µm Anotop filter

R_h (from Cumulant) = (3.9 ± 0.1) nm; R_h (from Regularization) = (4.0 ± 0.1) nm

Solution filtered through 0.2 µm Anotop filter

R_h (from Cumulant) = (4.9 ± 0.1) nm; R_h (from Regularization) = (4.0 ± 0.1) nm

Standard characterization data by Wyatt MALS detector following SEC separation (WTC-030S5 with PBS at 0.5 mL/min):

(Solution filtered through 0.02 µm Anotop filter)

Monomer% = 93.6 ± 0.1 ; M_w (including aggregates) = (74.8 ± 0.3) kDa

(Solution filtered through 0.2 µm Anotop filter)

Monomer% = 93.5 ± 0.1 ; M_w (including aggregates) = (77.4 ± 1.4) kDa

Certification: Sophia Kenrick

Date: 6/12/2019